

CERTIFICATION OF ANALYSIS

Product Name	Bacteriostatic Water	**Lot Number**	AYK20260531-BAC3
Appearance	Clear, colorless liquid	**Laboratory ID**	LB20260531-033
Main Component:	Sterile Water with 0.9% Benzyl Alcohol	**Manufacturing Date**	2026/05/28
Specification	3ml/vial	**Report Date**	2026/05/31

HPLC CHROMATOGRAM

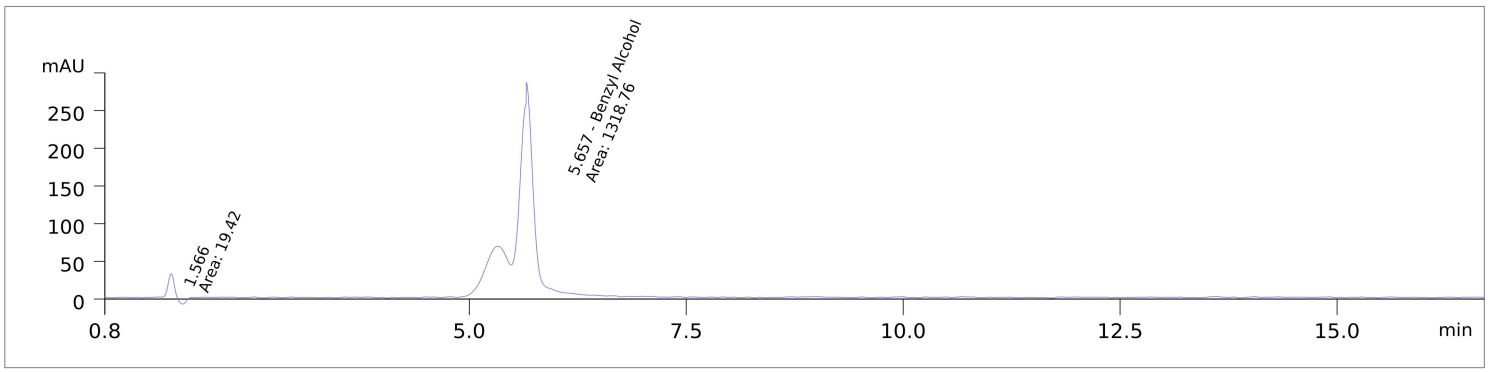

MASS IDENTIFICATION

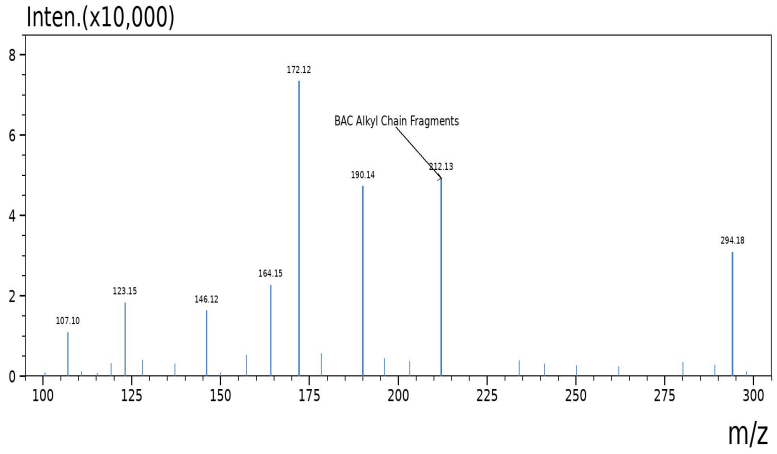

PRODUCT IMAGE



ANALYSIS RESULTS

Specification	Result	Method	Status
Identity:BAC Water	Positive for Benzyl Alcohol	HPLC -UV	√ Conforms
Content	0.92%w/v	HPLC Quantitation	√ Conforms
pH	5.86	pH Meter	√ Conforms

NOTES & DISCLAIMER

The analytical testing reported herein was conducted under controlled laboratory conditions using validated HPLC and LC-MS methodologies. The results presented are specific to the tested batch and may be influenced by storage conditions, sample handling, transportation, and other experimental variables. This certificate is intended for research and quality verification purposes only.

Analyzed By: wang kun

2026/05/31

Approved By HUANG YU

2026/05/31